NEXA™ NPWT System

WHAT HAPPENS WHEN THERE IS A LEAK?

AOTI

CONVENTIONAL AIR PUMP DEVICES

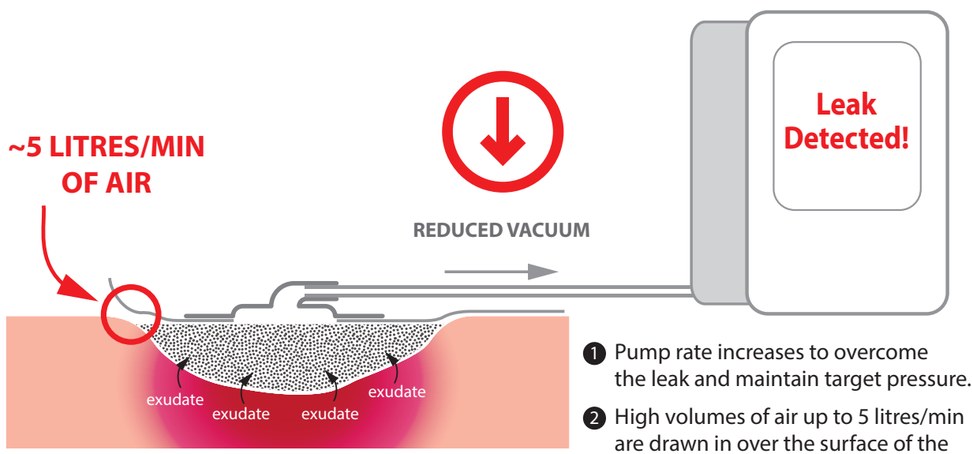

1. Pump rate increases to overcome the leak and maintain target pressure.
2. High volumes of air up to 5 litres/min are drawn in over the surface of the dressing.

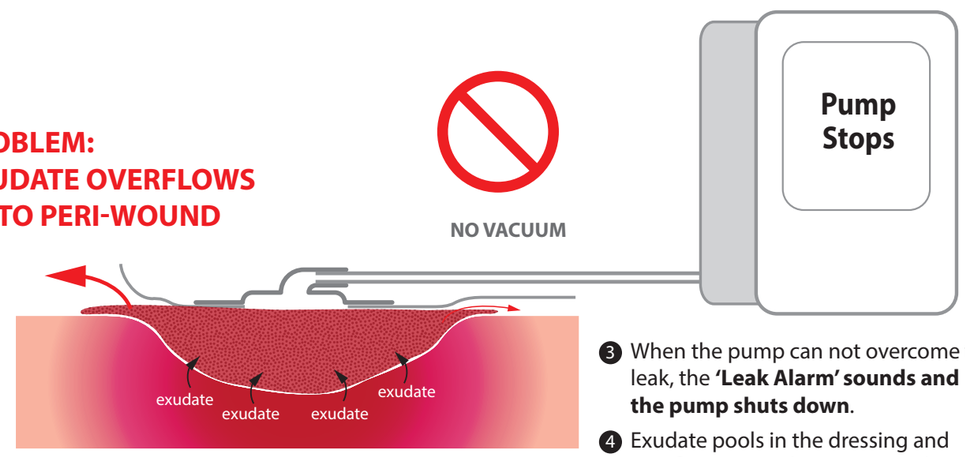

3. When the pump can not overcome the leak, the **'Leak Alarm' sounds and the pump shuts down**.
4. Exudate pools in the dressing and overflows on to the peri-wound **potentially causing maceration**.

NEXA™ NPWT System

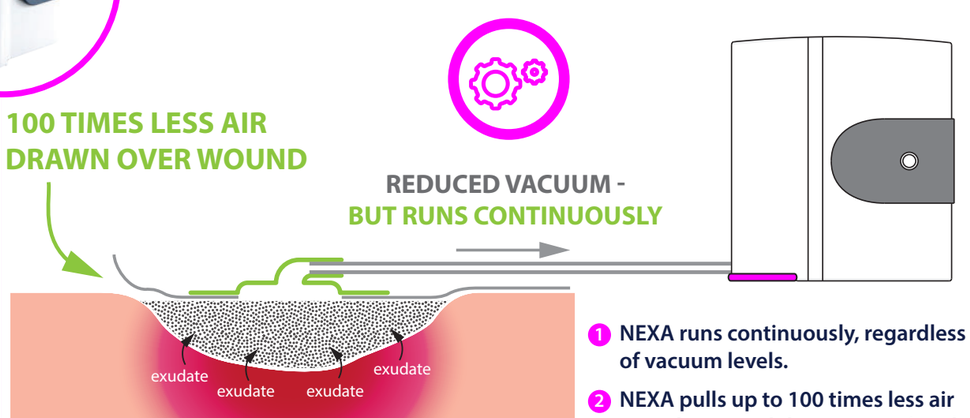

1. **NEXA runs continuously, regardless of vacuum levels.**
2. **NEXA pulls up to 100 times less air over the wound than conventional air pumps due to NEXA's hydrodynamic fluid pump technology.**

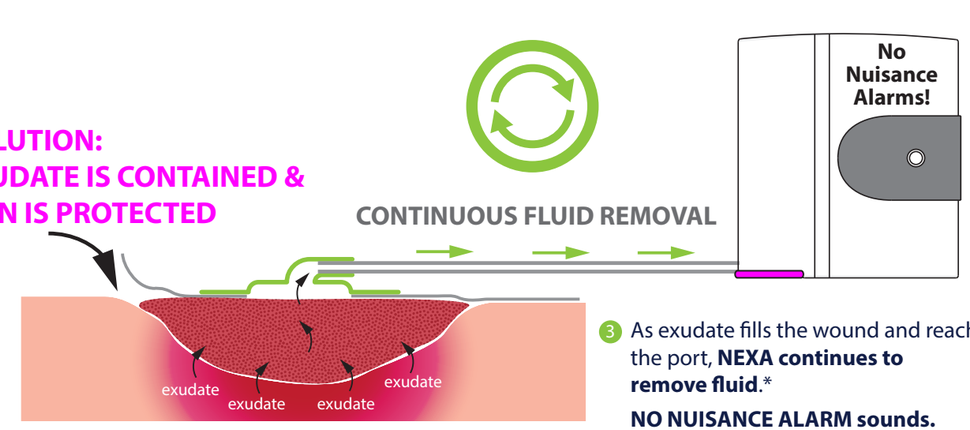

3. As exudate fills the wound and reaches the port, **NEXA continues to remove fluid**.*

NO NUISANCE ALARM sounds.

THIS REDUCES THE POTENTIAL FOR SKIN MACERATION

*Dressing leaks do not require immediate attention but should be addressed to ensure full benefit of therapy.

MB4002-B